

Methods of test for

Paints —

Part A9: Determination of flashpoint
(closed cup equilibrium method —

Flashpoint of petroleum and related products —

Part 2: Method for determination of
flashpoint (closed cup equilibrium
method) —

[ISO title: Paints, varnishes, petroleum
and related products —

Determination of flashpoint — Closed
cup equilibrium method]

UDC 667.612:536.468:543.873

Committees responsible for this British Standard

The preparation of this British Standard was entrusted by the Petroleum Standards Committee (PTC/-) and the Pigments, Paints and Varnishes Standards Committee (PVC/-) to Technical Committees PTC/13 and PVC/10, upon which the following bodies were represented:

- British Gas Corporation
- Chemical Industries Association
- Electricity Supply Industry in England and Wales
- Greater London Council
- Health and Safety Executive
- Institute of Metal Finishing
- Institute of Petroleum
- Ministry of Defence
- Oil and Colour Chemists' Association
- Paint Research Association
- Paintmakers Association of Great Britain Ltd.
- Titanium Pigment Manufacturers' Technical Committee
- Coopted member

This British Standard, having been prepared under the direction of the Petroleum Standards Committee and the Pigments, Paints and Varnishes Standards Committee, was published under the authority of the Board of BSI and comes into effect on 28 February 1986

© BSI 04-1999

First published, as BS 3900-A9, April 1973
First revision, jointly with BS 6664-2, February 1986

The following BSI references relate to the work on this standard:
Committee reference PTC/13 and PVC/10
Draft for comment 81/52418 DC

ISBN 0 580 14786 X

Amendments issued since publication

Amd. No.	Date of issue	Comments

Contents

	Page
Committees responsible	Inside front cover
National foreword	ii
0 Introduction	1
1 Scope and field of application	1
2 References	1
3 Definition	1
4 Principle	1
5 Apparatus	1
6 Sampling and sample treatment	2
7 Procedure	2
8 Calculation	3
9 Precision	3
10 Test report	4
11 Tests for referee purposes	4
Annex A Suitable closed cups specified in national standards	5
Annex B Sampling procedures	5
Figure — Closed cup, with fitted stirrer (see 5.1), immersed in the bath	4
Publications referred to	Inside back cover

National foreword

These Parts of BS 3900 and BS 6664 have been prepared under the direction of the Petroleum Standards Committee and the Pigments, Paints and Varnishes Standards Committee. They are identical with ISO 1523-1983 “*Paints, varnishes, petroleum and related products — Determination of flashpoint — Closed cup equilibrium method*”, published by the International Organization for Standardization (ISO). ISO 1523 was prepared as a result of discussions in ISO Technical Committee 28, Petroleum products and lubricants, and ISO Technical Committee 35, Paints and varnishes, in which the UK participated.

This Part of BS 3900 supersedes BS 3900-A9:1973, which is withdrawn. This revision contains only minor technical changes from the previous edition of BS 3900-A9, and it essentially constitutes an editorial revision to enable the test procedure which was applicable to paints, varnishes and related products to be equally applicable to petroleum and similar products. To ensure that this additional applicability is not overlooked by its publication within BS 3900, covering methods of test for paints, this standard is also published as Part 2 of BS 6664, covering flashpoint of petroleum and related products.

Initially BS 6664 will consist of four Parts which are identical with four international standards prepared jointly by ISO/TC 28 and ISO/TC 35, which correspond as follows:

International standard	Corresponding British Standard	
	BS 3900 Methods of test for paints	BS 6664 Flashpoint of petroleum and related products
ISO 1516:1981	Part A8:1986 Test for flash/no flash (closed cup equilibrium method)	Part 1:1986 Method of test for flash/no flash (closed cup equilibrium method)
ISO 1523:1983	Part A9:1986 Determination of flashpoint (closed cup equilibrium method)	Part 2:1986 Method for determination of flashpoint (closed cup equilibrium method)
	BS 3900 Methods of test for paints	BS 6664 Flashpoint of petroleum and related products
ISO 3679:1983	Part A14:1986 Determination of flashpoint (rapid equilibrium method)	Part 4:1986 Method for determination of flashpoint (rapid equilibrium method)
ISO 3680:1983	Part A13:1986 Test for flash/no flash (rapid equilibrium method)	Part 3:1986 Method of test for flash/no flash (rapid equilibrium method)

Additional Parts may eventually be added to BS 6664, if appropriate. Other British Standard methods for the determination of flashpoint¹⁾ of petroleum and related materials include the following:

- BS 2000, *Methods of test for petroleum and its products*.
- BS 2000-33, *Flash point by the Abel apparatus (Statutory method: Petroleum (Consolidation) Act 1928)*.
- BS 2000-34, *Flash point by Pensky-Martens closed tester*.
- BS 2000-35, *Flash point (open) and fire point of petroleum products by the Pensky-Martens apparatus*.

¹⁾ In this standard the term “flashpoint” has been used as a single word to maintain the identity with ISO 1523. In other British Standards such as BS 2000 and BS 4689 (identical with ISO 2592) the term has been used as two words. No difference is implied by this difference in usage which has arisen from the separate development of these two groups of standard.

BS 2000-113, *Flash point (closed) of cutback bitumen*.

BS 2000-170, *Flash point by the Abel apparatus (non-statutory method)*.

BS 4689, *Method for determination of flash and fire points to petroleum products: Cleveland open cup method*.

It has been assumed in the drafting of this British Standard that it will be used and applied by those who are appropriately qualified and experienced.

Terminology and conventions. The text of the international standard has been approved as suitable for publication as a British Standard without deviation. Some terminology and certain conventions are not identical with those used in British Standards; attention is drawn especially to the following.

The comma has been used throughout as a decimal marker. In British Standards it is current practice to use a full point on the baseline as the decimal marker.

Wherever the words "International Standard" appear, referring to this standard, they should be read as "British Standard" and wherever the identification "ISO 1523" appears it should be read as either "BS 3900-A9" or "BS 6664-2".

Cross-references

International standard	Corresponding British Standard
	BS 3900 Methods of test for paints
ISO 1512:1974	Part A1:1970 Sampling (Technically equivalent)
ISO 1513:1980	Part A2:1983 Examination and preparation of samples for testing (Identical)
ISO 1516:1981	Part A8:1986 ^a . Test for flash/no flash (closed cup equilibrium method) (Identical)
ISO 3170:1975 ^b	BS 3195 Methods for sampling petroleum products Part 1:1978 Liquid hydrocarbons — manual sampling (Identical)
ISO 3679:1983	BS 3900 Methods of test for paints Part A14:1986 ^c Determination of flashpoint (rapid equilibrium method) (Identical)

^a Also numbered as BS 6664-1 (see paragraph 3).

^b In revision.

^c Also numbered as BS 6664-4 (see paragraph 3).

There is no British Standard corresponding to ISO 3171:1975²⁾. The Technical Committee PTC/13 has reviewed the provisions of ISO 3171 to which reference is made in **B.2** and has decided that they are acceptable for use in conjunction with this standard.

With reference to Annex A, the British Standards referred to have been withdrawn and superseded by the following Parts of BS 2000 (see paragraph 4) which are technically equivalent to the withdrawn British Standards.

BS 3442 superseded by BS 2000-33 and BS 2000-170;

BS 2839 superseded by BS 2000-34.

²⁾ In revision.

Additional information. In using this standard as Part of BS 3900 it may be helpful to refer to the general information in the Introduction to BS 3900, issued separately.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i to iv, pages 1 to 6, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

0 Introduction

This International Standard describes one of two methods for the determination of the flashpoint of paints, varnishes, petroleum and related products and it should be read in conjunction with ISO 3679 when selecting a method.

By the procedure specified in this International Standard, differences between test apparatus of various standard designs are minimized by ensuring that the test is carried out only when the product under test and the air/vapour mixture above it in the test vessel are approximately in temperature equilibrium.

Nevertheless the interpretation of results obtained from solvent mixtures containing halogenated hydrocarbons should be considered with caution as these mixtures can give anomalous results³⁾.

NOTE The flash/no flash test using the same equipment under equilibrium conditions is given in ISO 1516.

1 Scope and field of application

This International Standard specifies a method for determining the flashpoint of a paint, varnish, paint binder, solvent, petroleum or a related product and makes allowance for deviations from standard atmospheric pressure.

The method is suitable for use over the temperature range 5 to 110 °C, although some of the apparatus listed in Annex A cannot cover all of this range using the thermometer supplied with the apparatus.

NOTE 1 In some countries, existing regulations may require the use of other methods over at least a part of the temperature range 5 to 110 °C.

NOTE 2 Care should be taken in the interpretation of results obtained from solvent mixtures containing halogenated hydrocarbons (see clause 0).

2 References

- ISO 1512, *Paints and varnishes — Sampling.*
- ISO 1513, *Paints and varnishes — Examination and preparation of samples for testing.*
- ISO 1516, *Paints, varnishes, petroleum and related products — Flash/no flash test — Closed cup equilibrium method.*
- ISO 3170, *Petroleum products — Liquid hydrocarbons — Manual sampling.*
- ISO 3171, *Petroleum products — Liquid hydrocarbons — Automatic pipeline sampling.*
- ISO 3679, *Paints, varnishes, petroleum and related products — Determination of flashpoint — Rapid equilibrium method.*

3 Definition

flashpoint (closed cup)

minimum temperature to which a product, confined in a closed cup, must be heated for the vapours emitted to ignite momentarily in the presence of a flame, when operating under standardized conditions

NOTE In this International Standard, the flashpoint is corrected to an atmospheric pressure of 101,3 kPa (1 013 mbar).

4 Principle

The test portion is heated in a suitably designed closed cup by immersing it to the required level in a suitable bath. The temperature of the bath is slowly raised at such a rate that the difference in temperature between the liquid in the bath and the test portion in the cup never exceeds 2 °C, and the heating procedure ensures that the temperature of the test portion does not rise more quickly than about 0,5 °C in 1,5 min (see note 1).

During the heating-up period, ignition trials are carried out at intervals of not less than 1,5 min (see note 2). The lowest temperature at which a flash occurs is noted and from this and a duplicate determination the flashpoint of the test product is calculated, corrected to the standard atmospheric pressure of 101,3 kPa (1 013 mbar).

NOTE 1 To ensure that the test is carried out under approximately equilibrium conditions, a slow rate of heating is necessary because of the low thermal conductivity of some products and also because heat transfer by convection is hindered by the high viscosity of many products. Uniformity of temperature throughout the product under test may be assisted by use of a stirring device, although it is **not** to be operated during an ignition trial.

NOTE 2 A minimum time interval of 1,5 min is necessary to ensure that a saturation concentration of vapour in the air space above the test portion is re-established after each ignition trial.

5 Apparatus

5.1 Test cup. A closed cup with an internal level indicator; the closed cups specified in a number of national standards (see Annex A) satisfy the necessary requirements. If a stirrer is fitted to the test cup used, it may be operated during the heating-up period but shall be stopped during the ignition trial. If a stirrer originally fitted to the test cup is removed, the aperture in the cover shall be securely plugged before starting the test.

³⁾ RYBICKY, J. and STEVENS, J.R., *J. Coatings Technol.* **53** (676) May 1981:40-42.

Essentially, the test cup shall be fitted with a cover which carries an opening slide and an ignition device which is inserted to a prescribed level into one of the openings in the cover when a test is made. The details of the cover, slide, ignition device and its movement shall be in accordance with the appropriate national standard listed in Annex A. The equipment is such that an ignition trial can be performed by opening the slide, inserting and removing the nozzle of the ignition device, and closing the slide again, in a period of $2,5 \pm 0,5$ s. A mechanically driven device for the opening of the slide and applying the ignition device to the air/vapour mixture in the cup is permissible and the source of flame for the ignition device may be any suitable flammable gas.

5.2 Bath, containing a suitable liquid, capable of being adjusted to the required temperature (see **7.2.1.2**) and of adequate heat capacity to meet the requirements of **7.2.3.6**. A bath fitted with a stirrer and thermostat of suitable range is convenient. Other procedures for heating the closed cup may be used if the rate of heating complies with the requirements given in clause 4.

5.3 Thermometers.

The test cup (**5.1**) shall be fitted with a thermometer of appropriate range and dimensions that, when immersed in the test portion, measures its temperature with an error no greater than $0,5^\circ\text{C}$. A thermometer having a graduation at each $0,5^\circ\text{C}$ is recommended.

The bath (**5.2**) shall be fitted with a thermometer of equal precision.

When required, the accuracy of the thermometers shall be checked against a reference standard by an authorized laboratory using the stipulated immersion.

5.4 Support, for holding the test cup in the bath (**5.2**) so that the cover and upper edge are horizontal. The cup is immersed in direct contact with the liquid in the bath in such a position that the level of the test portion in the cup is the same as that of the liquid in the bath (see the Figure).

6 Sampling and sample treatment

6.1 Take a representative sample of the product to be tested using the appropriate sampling procedure for the product concerned. References to sampling procedures for various products are given in Annex B.

The sample shall be kept in an airtight container until it is to be tested. The ullage, i.e. the air space above the contents of the container, shall not be more than 10 % of the total capacity of the container.

Samples shall not be stored in plastics (polyethylene, polypropylene, etc.) bottles.

6.2 Because of the possibility of loss of volatile constituents, the sample container shall be cooled to at least 10°C below the expected flashpoint before opening it to remove the test portion. The sample shall receive only the minimum mixing treatment to ensure uniformity. After removal of the test portion, the sample container shall immediately be tightly closed to ensure that loss of volatile components from the container is minimized. If this is not carried out, the product sample shall be deemed unsuitable for further testing.

7 Procedure

7.1 Preliminary test

Determine the approximate flashpoint of the sample by one or more preliminary tests. This determines the starting temperature for the definitive test, which shall be about 5°C below the expected value.

7.2 Definitive test

7.2.1 Preparation of apparatus

7.2.1.1 Set up the apparatus in a draught-free position and preferably in subdued light.

7.2.1.2 Adjust the temperature of the liquid in the bath (**5.2**) to 5°C below the approximate flashpoint as determined according to **7.1**.

7.2.1.3 Carefully clean and dry the test cup (**5.1**), its cover and thermometer (**5.3**). Bring them to approximately the same temperature as the bath in **7.2.1.2**.

7.2.2 Test portion

7.2.2.1 Obtain and prepare the test portion in accordance with clause **6**, and ensure that at all times during this preparation its temperature is at least 10°C below the expected flashpoint temperature.

7.2.2.2 Fill the cup with the test portion until the internal level indicator just disappears under the surface of the liquid. Take care to avoid both the formation of bubbles and contact between the sample and the cup wall above the level indicator. If either of these conditions occurs to a significant extent, empty the cup, prepare it again according to **7.2.1.3**, and fill it with a fresh test portion.

7.2.3 Determination

7.2.3.1 Immediately after filling the cup, place the cover and thermometer in position. Support the cup in the bath so that the cover is horizontal and the cup is immersed in direct contact with the liquid in the bath and with the surface of the test portion at the same level as that of the liquid in the bath. Confirm that the bath is at the required temperature as defined in **7.2.1.2**.

7.2.3.2 Light the flame of the ignition device and adjust it to an approximately spherical shape of diameter $3,5 \pm 0,5$ mm.

7.2.3.3 As soon as the test portion has attained the same temperature as the liquid in the bath (i.e. the starting temperature of the definitive test), perform an ignition trial by opening the slide, inserting and removing the nozzle of the ignition device, and closing the slide again, over a period of $2,5 \pm 0,5$ s. Watch for a flash between opening and closing the slide.

7.2.3.4 Record whether a flash has occurred.

NOTE When the vapour mixture under test is near the flashpoint, application of the ignition flame may give rise to a halo; however, the product is only deemed to have flashed if a comparatively large blue flame appears and propagates itself over the surface of the liquid.

If a large blue flame does not appear as a flash, but instead a continuous luminous flame burns in the orifice when the slide is opened and the ignition flame is introduced, then the flashpoint of the product lies considerably below the test temperature and therefore the preliminary test (7.1) should be repeated at a temperature of at least 10°C below the expected flashpoint.

7.2.3.5 If a flash occurs (see the note to **7.2.3.4**), carry out the procedure (**7.2.3**) again with a fresh test portion but starting the test at a temperature about 5°C lower than that selected previously.

7.2.3.6 If no flash occurs (see the note to **7.2.3.4**), heat the bath at a rate such that the difference in temperature between the bath and the test portion never exceeds 2°C . When the test portion has increased in temperature by $0,5^\circ\text{C}$ (i.e. after not less than 1,5 min), repeat the ignition test and if no flash is observed repeat the procedure until a temperature is reached at which a flash occurs (see note). Read to the nearest $0,5^\circ\text{C}$ the temperature indicated by the cup thermometer, correct this reading for any known thermometer correction, and record the result as the flashpoint at the atmospheric pressure prevailing during the test. Record also the atmospheric pressure in kilopascals, millibars, or millimetres of mercury.

NOTE As volatile components are likely to be present in the products to be tested, the total duration of the test should not exceed 1 h.

7.2.4 Replicate determination

7.2.4.1 Clean the cup and carry out a second determination using a fresh test portion and repeating the procedures described in **7.2.1** to **7.2.3**. Calculate the mean corrected flashpoint (see clause 8) to the nearest $0,5^\circ\text{C}$.

7.2.4.2 For referee tests where a better level of precision is required, the procedure specified in clause 11 should be followed.

8 Calculation

Calculate the flashpoint, in degrees Celsius, corrected to standard atmospheric pressure of 101,3 kPa (1 013 mbar or 760 mmHg), by adding algebraically to the observed temperature the correction from one of the following equations

$$C = \frac{101,3 - p_0}{4} \text{ or } \frac{1013 - p_1}{40} \text{ or } \frac{760 - p_2}{30}$$

where

- C is the correction, in degrees Celsius;
- p_0 is the atmospheric pressure, expressed in kilopascals;
- p_1 is the atmospheric pressure, expressed in millibars;
- p_2 is the atmospheric pressure, expressed in millimetres of mercury.

Record the mean corrected flashpoint to the nearest $0,5^\circ\text{C}$.

NOTE Whilst these formulae are strictly correct only within the barometric pressure range from 98,0 to 104,7 kPa, for pressures outside this range the error is sufficiently small to be ignored.

9 Precision

9.1 Repeatability (r)

The value below which the absolute difference between two single test results obtained on identical material by one operator in one laboratory using the same equipment within a short interval of time using the standardized test method, may be expected to lie with a 95 % probability, is 2°C .

9.2 Reproducibility (R)

The value below which the absolute difference between the mean of two single test results obtained on identical material by operators in different laboratories, using the standardized test method, may be expected to lie with a 95 % probability, is 3°C .

10 Test report

The test report shall include at least the following information:

- the type and identification of the product tested;
- a reference to this International Standard (ISO 1523);
- a reference to the standard describing the test cup used, and details of any modifications made;
- the mean corrected flashpoint, in degrees Celsius, calculated as in clause 8;
- any deviation, by agreement or otherwise, from the test procedure specified;
- the date of the test.

11 Tests for referee purposes


11.1 For referee tests, more than two individual measurements may be required to achieve the necessary agreement.

11.2 If the difference between the results of two individual tests, calculated in accordance with clause 8, does not exceed $1,0^{\circ}\text{C}$, report the mean value to the nearest $0,5^{\circ}\text{C}$ as the flashpoint.

11.3 If the difference between the first two results exceeds $1,0^{\circ}\text{C}$ a third test shall be made. If the greatest difference between the three results does not exceed $1,5^{\circ}\text{C}$, report the mean value to the nearest $0,5^{\circ}\text{C}$ as the flashpoint.

11.4 If the greatest difference between the first three results exceeds $1,5^{\circ}\text{C}$, two further tests shall be made. If only one of the five results differs by more than $1,5^{\circ}\text{C}$ from the mean value, reject this result and report the mean value of the other four results to the nearest $0,5^{\circ}\text{C}$ as the flashpoint.

11.5 If more than one of the five results differ by more than $1,5^{\circ}\text{C}$ from the mean value, report this mean value to the nearest $0,5^{\circ}\text{C}$ as the flashpoint but state also the individual values and add a note to the test report on the irregular flashing of the product tested.

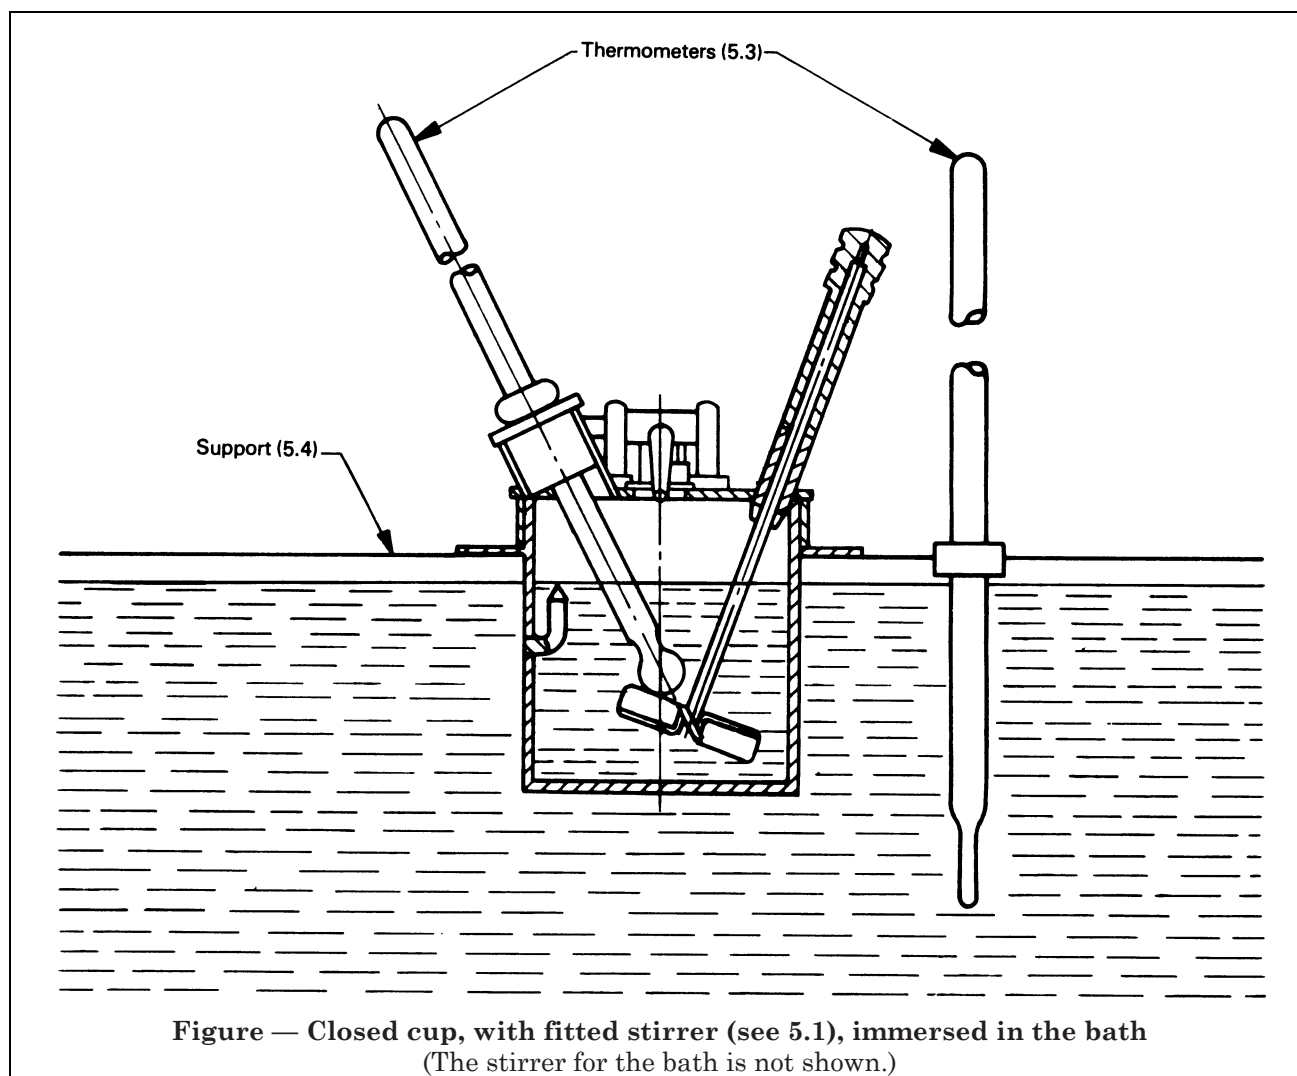

Annex A Suitable closed cups specified in national standards

The cups listed below of closed-cup apparatus described in standards are known to satisfy the necessary requirements of this method of test for the determination of flashpoint. The method requires immersion of the cup in a bath and if a suitable bath is not included in the standard apparatus one must be provided (see 5.2).

Abel cup	French Standard	NF T 66-009
Abel cup	French Standard	NF M 07-011
^a Abel cup	British Standard	BS 3442 (and IP 33 and IP 170)
Abel-Pensky cup	Czechoslovak Standard	CSN 67 3015
Abel-Pensky cup	French Standard	NF M 07-036
Abel-Pensky cup	German Standard	DIN 51 755
Abel-Pensky cup (+ stirrer)	Swedish Standard	SIS 02 18 11
Abel-Pensky cup (modified according to Bleisch)	German Standard	DIN 53 213 Teil 1
Pensky-Martens cup	International Standard	ISO 2719
^a Pensky-Martens cup	British Standard	BS 2839 (and IP 34)
Pensky-Martens cup	French Standard	NF M 07-019
Pensky-Martens cup	German Standard	DIN 51 758
Pensky-Martens cup	Netherlands Standard	NEN-ISO 2719
Pensky-Martens cup	Swedish Standard	SIS 02 18 12
Pensky-Martens cup	USA Standard	Z 11.7 (and ASTM D 93)
Tag cup	USA Standard	Z 11.24 (and ASTM D 56)

^a See national foreword.

Annex B Sampling procedures

B.1 Paints, varnishes and related products

Take a representative sample of the product to be tested as described in ISO 1512 and examine and prepare it for testing as described in ISO 1513. In addition observe the precautions of clause 6 and 7.2.2.1.

B.2 Petroleum and related products

Take a representative sample of the product to be tested as described in ISO 3170 or ISO 3171 as appropriate. In addition observe the precautions of clause 6 and 7.2.2.1.

Publications referred to

See national foreword.

BS 3900-A9:
1986
BS 6664-2:
1986
ISO 1523:1983

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.

BSI
389 Chiswick High Road
London
W4 4AL