

## Methods of test for paints

# Part B12: Determination of “soluble” mercury content

[ISO title: Paints and varnishes — Determination of “soluble” metal content — Part 7: Determination of mercury content of the pigment portion of the paint and of the liquid portion of water-dilutable paints — Flameless atomic absorption spectrometric method]

It is recommended that this Part be read in conjunction with the general information in the Introduction to BS 3900, issued separately

UDC 667.61:620.1

This British Standard, having been prepared under the direction of the Pigments, Paints and Varnishes Standards Committee, was published under the authority of the Board of BSI and comes into effect on 31 January 1986

© BSI 07-1999

The Committees responsible for this British Standard are shown in BS 3900: Introduction

The following BSI references relate to the work on this standard:  
Committee reference PVC/10  
Draft for comment 82/55556 DC

ISBN 0 580 14951 X

Amendments issued since publication

Amd. No.	Date of issue	Comments

# Contents

	Page
National foreword	ii
0 Introduction	1
1 Scope and field of application	1
2 References	1
3 Principle	1
4 Reagents and materials	1
5 Apparatus	2
6 Procedure	2
7 Expression of results	4
8 Test report	5
Figure 1 — Firing adapter	6
Figure 2 — Example of apparatus for the determination of mercury by flameless atomic absorption spectrometry	7
Figure 3 — General view of the combustion apparatus	8
Publications referred to	Inside back cover

# National foreword

This Part of BS 3900 has been prepared under the direction of the Pigments, Paints and Varnishes Standards Committee. It is identical with ISO 3856-7:1984 *“Paints and varnishes — Determination of “soluble” metal content”* Part 7: *“Determination of mercury content of the pigment portion of the paint and of the liquid portion of water-dilutable paints — Flameless atomic absorption spectrometric method”* published by the International Organization for Standardization (ISO).

It is assumed in the drafting of this standard that it will be used and applied by those who are appropriately qualified and experienced. The procedures described in this standard are intended to be carried out by suitably trained and/or supervised personnel. The substances and procedures described may be injurious to health if inadequate precautions are taken. This standard refers only to its technical suitability and does not absolve the user from statutory obligations relating to health and safety.

**Terminology and conventions.** The text of the international standard has been approved as suitable for publication as a British Standard without deviation. Some terminology and certain conventions are not identical with those used in British Standards; attention is drawn especially to the following.

The comma has been used as a decimal marker. In British Standards, it is current practice to use a full point on the baseline as the decimal marker.

In British Standards it is current practice to use the symbol “L” for litre rather than “l”, and to use the spelling “sulphur”, etc., instead of “sulfur”, etc.

Wherever the words “International Standard” and “part of ISO 3856” appear, referring to this standard, they should be read as “British Standard” and “Part of BS 3900” respectively, and wherever the identification “ISO 3856-7” appears, it should be read as “BS 3900-B12”.

## Cross-references

International standards	Corresponding British Standards
ISO 1042:1983	BS 1792:1982 <i>Specification for one-mark volumetric flasks</i> (Identical)
ISO 6713:1984	BS 3900 <i>Methods of test for paints</i> <i>Part B5:1986 Preparation of acid extracts from liquid paints or coating powders</i> (Identical)

The Technical Committee has reviewed the provisions of ISO 385-1:1984, and ISO 648:1977 to which reference is made in the text, and has decided that they are acceptable for use in conjunction with this standard. ISO 385-1 is related to BS 846 *“Specification for burettes”* and ISO 648 is related to BS 1583 *“One-mark pipettes”*.

The Technical Committee has reviewed the proposed provisions of ISO 3696 to which reference is made in clause 4 and has decided that they are acceptable for use in conjunction with this standard. ISO 3696 is related to BS 3978 *“Water for laboratory use”*.

ISO 3856, to which reference is made in clause 0, is published in a number of Parts of BS 3900. At the time of publication of this standard, the relationship between other Parts of BS 3900 and Parts of ISO 3856 was as follows:

Part of ISO 3856	Corresponding Part of BS 3900
	BS 3900 <i>Methods of test for paints</i>
ISO 3856-1:1984	<sup>a</sup> Part B6:1986 <i>Determination of “soluble” lead content</i> (Identical)
ISO 3856-2:1984	Part B7:1986 <i>Determination of “soluble” antimony content</i> (Identical)
ISO 3856-3:1984	Part B8:1986 <i>Determination of “soluble” barium content</i> (Identical)
ISO 3856-4:1984	Part B9:1986 <i>Determination of “soluble” cadmium content</i> (Identical)
ISO 3856-5:1984	Part B10:1986 <i>Determination of hexavalent chromium content of solid matter</i> (Identical)
ISO 3856-6:1984	Part B11:1986 <i>Determination of total chromium content of liquid matter</i> (Identical)

<sup>a</sup> Attention is drawn to a similar standard, BS 3900-B3 “*Determination of “soluble” lead in the solid matter in liquid paints*”: method for use in conjunction with The Control of Lead at Work Regulations, 1980 (S.I. 1980 No. 1248)”.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, pages i to iv, pages 1 to 8, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.



## 0 Introduction

This International Standard is a part of ISO 3856, *Paints and varnishes — Determination of “soluble” metal content*.

## 1 Scope and field of application

This part of ISO 3856 describes a flameless atomic absorption spectrometric method for the determination of the mercury content of the test solutions, prepared according to ISO 6713 or other suitable International Standards.

The method is applicable to paints having “soluble” mercury contents in the range of about 0,005 to 0,05 % (m/m), but the part of this method covering the examination of the liquid portion of the paint is restricted to water-dilutable paints.

**CAUTION — The procedures described in this part of ISO 3856 are intended to be carried out by qualified chemists or by other suitably trained and/or supervised personnel. The substances and procedures used in this method may be injurious to health if adequate precautions are not taken. Attention is drawn in the text (see 4.6 and 4.7) to certain specific hazards. This part of ISO 3856 refers only to its technical suitability and does not absolve the user from statutory obligations relating to health and safety.**

## 2 References

ISO 385-1, *Laboratory glassware — Burettes — Part 1: General requirements*<sup>1)</sup>.

ISO 648, *Laboratory glassware — One-mark pipettes*.

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*.

ISO 3696, *Water for laboratory use — Specifications*<sup>2)</sup>.

ISO 6713, *Paints and varnishes — Preparation of acid extracts from paints in liquid or powder form*.

## 3 Principle

Oxidation of the mercury compounds contained in the test solution obtained from the pigment portion of the paint or combustion with oxygen in an enclosed system of the evaporation residue of the test solution obtained from the liquid portion of water-dilutable paints.

Reduction of the mercury(II) compounds contained in the resulting solutions to elementary mercury. Entrainment of the mercury in a current of gas at ambient temperature and determination of the mercury, as the monoatomic vapour, by cold vapour (flameless) atomic absorption spectrometry at a wavelength in the region of 253,7 nm.

## 4 Reagents and materials

During the analysis, use only reagents of recognized analytical grade and water of at least grade 3 purity according to ISO 3696.

**4.1 Oxygen**, commercial grade, in a steel cylinder.

**4.2 Tin(II) chloride dihydrate**, 100 g/l solution.

Dissolve 25 g of tin(II) chloride dihydrate ( $\text{SnCl}_2 \cdot 2\text{H}_2\text{O}$ ) in 50 ml of 35 % (m/m) (ρ approximately 1,18 g/ml) hydrochloric acid and dilute to 250 ml with water. Add a few granules of metallic tin and heat until any precipitate disappears. Ensure that a few granules of bright tin are present to stabilize the solution and, before use, that there is no precipitate.

**4.3 Sulfuric acid**, 5 % (m/m).

**4.4 Nitric acid**, approximately 65 % (m/m) (ρ approximately 1,40 g/ml).

**4.5 Potassium permanganate**, 60 g/l solution.

Dissolve 60 g of potassium permanganate ( $\text{KMnO}_4$ ) in water and dilute to 1 litre.

**4.6 Hydroxylammonium chloride**, 20 % (m/m) solution.

**WARNING — Hydroxylammonium chloride is toxic, corrosive and an irritant. Avoid contact with eyes and skin.**

Dissolve 20 g of hydroxylammonium chloride ( $\text{NH}_2\text{OHCl}$ ) in about 75 ml of water and dilute to 100 ml.

**4.7 Mercury**, standard stock solution containing 100 mg of Hg per litre.

**WARNING — Mercury, particularly in its vapour form, and its solutions are toxic. Avoid breathing mercury vapour. Avoid contact of mercury or its solutions with eyes and skin. Carry out all procedures in a well-ventilated fume cupboard.**

Either

- a) transfer the contents of an ampoule of a standard mercury solution containing exactly 0,1 g of Hg into a 1 000 ml one-mark volumetric flask, dilute to the mark with the 5 % (m/m) sulfuric acid (4.3) and mix well;

<sup>1)</sup> At present at the stage of draft. (Partial revision of ISO/R 385:1964.)

<sup>2)</sup> At present at the stage of draft.

or

b) weigh, to the nearest 0,1 mg, 0,135 4 g of mercury(II) chloride, dissolve in the sulfuric acid (4.3) in a 1 000 ml one-mark volumetric flask, dilute to the mark with the same sulfuric acid and mix well.

1 ml of this standard stock solution contains 0,1 mg of Hg.

**4.8 Mercury**, standard solution containing 1 mg of Hg per litre.

Prepare this solution on the day of use.

Pipette 10 ml of the standard stock solution (4.7) into a 1 000 ml one-mark volumetric flask, dilute to the mark with the sulfuric acid (4.3) and mix well.

1 ml of this standard solution contains 1 µg of Hg.

## 5 Apparatus

Ordinary laboratory apparatus and

**5.1 Atomic absorption spectrometer**, suitable for measurements at a wavelength of 253,7 nm and capable of operating with the measuring cell specified in 5.2.

NOTE If special commercial mercury analyzers using the cold vapour AAS principle are used (see note to 6.1.2.1), appropriate amendment of the procedure described in 6.1.2 and 6.3.2 may be necessary and this should be recorded in the test report.

**5.2 Measuring cell**, with windows (for example of quartz) transparent to ultraviolet radiation (in the region of 253,7 nm), the optical path length of which should be appropriate to the spectrometer being used, but not less than 100 mm.

**5.3 Mercury hollow-cathode lamp or mercury discharge lamp.**

**5.4 Potentiometric chart recorder.**

NOTE A suitable peak measuring device such as an electronic integrator may be used as an alternative.

**5.5 Combustion flask or separating funnel**, of capacity 500 ml, with a ground-glass joint.

**5.6 Test portion holder** (platinum gauze combustion basket) and **firing adapter**, suitable for fitting to the combustion flask (5.5) (see Figure 1).

**5.7 Spark generator**

NOTE A high-frequency vacuum tester has been found to be satisfactory.

**5.8 Flowmeter**, fitted with a stainless steel needle valve and capable of measuring flow rates within the range 0,4 to 3 l/min.

**5.9 Pump**, diaphragm type, capable of giving controlled air flow rates of 0,4 to 3 l/min, or *cylinder of compressed air* or *nitrogen* equipped with a suitable pressure regulating valve.

**5.10 Reaction vessel**, comprising a test tube, of capacity 25 ml, with a ground-glass joint neck to fit an interchangeable head and a four-way stopcock (see Figure 2).

**5.11 Equipment**, to prevent any condensation of water vapour in the measuring cell. Any appropriate system may be used for this purpose (for example an infra-red lamp, a black electrical heating element, or a rod heater).

**5.12 Flexible acid-resistant tubing** (for example silicone rubber tubing), suitable for connecting the apparatus (see Figure 2).

**5.13 Capsules**, of hardened gelatine, pharmaceutical grade.

**5.14 Rotary evaporator**, water cooled, capable of operation under vacuum with a rotation rate of 150 r/min.

**5.15 Water-bath**, capable of being maintained at  $45 \pm 5^\circ\text{C}$ .

**5.16 Burettes**, of capacity 10 ml and 25 ml, complying with the requirements of ISO 385-1.

**5.17 One-mark volumetric flasks**, of capacity 25 ml, 100 ml and 500 ml, complying with the requirements of ISO 1042.

**5.18 Pipettes**, of capacity 1 ml, 5 ml and 25 ml, complying with the requirements of ISO 648.

**5.19 Balance**, capable of weighing to 0,1 mg.

## 6 Procedure

### 6.1 Preparation of the calibration graph

#### 6.1.1 Preparation of the standard matching solutions

Prepare these solutions on the day of use.

Into a series of six 25 ml one-mark volumetric flasks (5.17), introduce from the 10 ml burette (5.16), respectively, the volumes of the standard mercury solution (4.8) shown in the following table, dilute each to the mark with the sulfuric acid (4.3) and mix well.

Standard matching solution No.	Volume of the standard mercury solution (4.8)	Corresponding concentration of Hg in the standard matching solution
	ml	µg/ml
0 <sup>a</sup>	0	0
1	1	0,04
2	2	0,08
3	3	0,12
4	4	0,16
5	5	0,20

<sup>a</sup> Blank matching solution.



### 6.1.2 Spectrometric measurement

**6.1.2.1** Install the measuring cell (5.2) and the mercury spectral source (5.3) in the spectrometer (5.1) and optimize the conditions for the determination of mercury. Adjust the instrument in accordance with the manufacturer's instructions and adjust the monochromator to the region of 253,7 nm in order to obtain the maximum absorbance. Connect the flowmeter (5.8), pump (5.9), reaction vessel (5.10) and measuring cell (5.2) with the minimum lengths of flexible tubing (5.12) as shown in Figure 2.

NOTE A closed-circuit measuring system may be used in which the mercury is recirculated by means of a pump. This will be particularly effective when the release of mercury vapour is delayed by interfering substances, e.g. bromide ions.

**6.1.2.2** Switch on the pump and move the four-way stopcock to the by-pass position. Adjust the needle valve or open the gas regulating valve to give a suitable flow rate (for example 1 l/min). Set the potentiometric chart recorder (5.4) to the appropriate range. Adjust the zero of the recorder to a suitable position on the chart and check for baseline drift and noise level (see 6.1.2.4).

**6.1.2.3** Disconnect the reaction vessel and, using a pipette (5.18), place 5 ml of the standard matching solution No. 5 into the vessel. Add by means of a pipette (5.18) 1 ml of the tin(II) chloride solution (4.2), mix well and immediately reconnect the reaction vessel. Reverse the four-way stopcock to allow the liberated mercury vapour to be swept through the measuring cell.

**6.1.2.4** A peak will be indicated on the recorder chart and, by means of the potentiometer and flow range controls, adjust the height of the peak on the chart to about one-half the full-scale reading. Ensure that a sharp peak is obtained. Repeat if a further check of the adjustment is required.

Return the stopcock to the by-pass position and repeat the procedure using 5 ml aliquot portions of the remaining standard matching solutions.

NOTE It may be necessary to repeat the initial test several times using the standard matching solution No. 5 in order to optimize the characteristics of the system.

### 6.1.3 Calibration graph

Plot a graph having the masses, in micrograms, of Hg contained in 1 ml of the standard matching solutions as abscissae and the corresponding peak heights or, more precisely, the peak areas (for example, the products of the peak height and the peak width at half the peak height), reduced by the value for the blank matching solution, as ordinates.

Over this range the curve should deviate only slightly from linearity.

NOTE Contamination of any portion of the apparatus with aromatic solvents may give false high results owing to absorption in the region of 254 nm.

## 6.2 Test solutions

### 6.2.1 Pigment portion of the liquid paint and paint in powder form

**6.2.1.1** Use the solutions obtained by the procedure described in sub-clause 8.2.3 of ISO 6713.

Carry out the following oxidation procedure in duplicate.

Pipette a 5 ml aliquot portion of each test solution into individual 100 ml one-mark volumetric flasks (5.17). Add to each flask, 50 ml of the sulfuric acid (4.3), followed by 10 ml of the potassium permanganate solution (4.5). Allow to stand for a minimum of 2 h or preferably overnight to ensure that the mercury is present as Hg(II). After this period, add 2 ml of the hydroxylammonium chloride solution (4.6) and mix gently to obtain a clear, almost colourless solution. Dilute to the mark with the sulfuric acid (4.3) and mix well.

Retain these solutions for the determination of the mercury content of the pigment portion of the paint.

**6.2.1.2** Carry out the procedure described in 6.2.1.1 in duplicate on 5 ml aliquot portions taken from the blank test solution obtained by the procedure described in sub-clause 8.4 of ISO 6713.

Retain these solutions as the blank test solutions for the pigment portion of the paint.

### 6.2.2 Liquid portion of the paint

NOTE The following procedure should be carried out only if the liquid portion has been obtained from a water-dilutable paint.

**6.2.2.1** Combine the liquid portions obtained according to sub-clause 6.4.2 (method B) of ISO 6713, using acetone, preferably, for all extractions. Make up to a total volume of 500 ml with acetone in a one-mark volumetric flask and mix well.

NOTE For paints with a high pigment content, it may not be necessary to extract such a large amount of paint and in these cases the total volume of liquors will be considerably less than 500 ml. If this is so, it will be acceptable to make up to a smaller total volume, but it will be necessary to adjust correspondingly the aliquot portion taken for the test and the calculation (see 7.1.2).

**6.2.2.2** Pipette 25 ml of the combined liquors (6.2.2.1) into a tared 100 ml round-bottomed flask having a ground-glass neck which fits the rotary evaporator (5.14). Fit the flask on to the rotary evaporator and adjust the speed to about 150 r/min. To increase the rate of evaporation, place a water-bath (5.15) maintained at  $45 \pm 5$  °C under the flask and continue the evaporation until no volatile solvents remain. Remove the flask from the evaporator, dry the outside with a clean tissue and reweigh the flask to determine the mass of non-volatile residue.

NOTE Application of vacuum to the rotary evaporator may be necessary to facilitate the removal of higher boiling solvents.

**6.2.2.3** Carry out the following procedure in duplicate.

Place a test portion of approximately 20 mg of the residue (**6.2.2.2**) in a tared gelatine capsule (**5.13**) and close immediately. Weigh the capsule and test portion to the nearest 0,1 mg.

Place the weighed capsule in the test portion holder (**5.6**) (see Figure 1). Fill the combustion flask (**5.5**) with the oxygen (**4.1**) at atmospheric pressure, quickly introduce from a 10 ml burette (**5.16**) 3 ml of the nitric acid (**4.4**) and insert the test portion holder making a gas tight seal at the ground-glass joint. Attach the spark generator (**5.7**) to the electrical leads of the test portion holder (see Figure 3), place the apparatus behind a safety screen and switch on the high voltage to activate the spark and ignite the test portion.

After combustion is complete, shake the flask and contents and allow to stand for 30 min with occasional shaking. Remove the test portion holder and add to the flask 22 ml of water from a 25 ml burette (**5.16**). Replace the test portion holder and shake thoroughly.

Retain the bulk of the contents of the combustion flask in a stoppered glass container of capacity approximately 25 ml.

**6.2.2.4** Pipette a 5 ml aliquot portion of each solution obtained from **6.2.2.3** into individual 100 ml one-mark volumetric flasks (**5.17**), dilute to the mark with the sulfuric acid (**4.3**) and mix well.

Retain these solutions for the determination of the mercury content of the liquid portion of the paint.

**NOTE** As a result of the previous combustion of the test portion, it is unnecessary at this stage to oxidize with potassium permanganate.

**6.2.2.5** Carry out rotary evaporation of a 25 ml portion of the acetone used to make up the combined liquid portions in **6.2.2.1**. Retain this as the blank test solution for the liquid portion of the paint.

**NOTE** Good quality redistilled solvent should be completely mercury-free and if this is used the procedure given in **6.2.2.5** may be omitted. If a residue is obtained following rotary evaporation it will be necessary to prepare a blank test solution as described in **6.2.2.1**, **6.2.2.3** and **6.2.2.4**.

### 6.2.3 Other test solutions

Use the test solutions obtained by other specified or agreed procedures. Carry out the procedure described in **6.2.1.1** including the oxidation process if the mercury has to be converted to Hg(II).

Prepare blank test solutions using the identical procedure but omitting the test solution.

## 6.3 Determination

**6.3.1** Carry out the determination for each test solution (**6.2.1.1**, **6.2.2.4** or **6.2.3**).

**6.3.2** Measure with a pipette a volume of the solution (**6.3.1**) into the reaction vessel (**5.10**) such that its peak reading will lie on the ordinate of the calibration graph. Add by means of a pipette (**5.18**) 1 ml of the tin(II) chloride solution (**4.2**), mix well and immediately reconnect the reaction vessel. Reverse the four way stopcock to allow the liberated mercury vapour to be swept through the measuring cell.

Record the peak reading (i.e. either peak height or peak area; see **6.1.3**), reduced by the reading obtained for the blank test solution. Read the mercury concentration from the calibration graph.

If the response of a test solution is higher than that of the standard matching solution with the highest mercury concentration (that is matching solution No. 5), dilute the test solution appropriately (dilution factor  $F$ ) with a known volume of the sulfuric acid (**4.3**) before repeating the determination.

**6.3.3** Carry out a blank test immediately after the determination, following the same procedure, using the solution obtained in **6.2.1.2**, **6.2.2.5** or **6.2.3**, as appropriate.

**6.3.4** Calculate the mean of the duplicate readings. If the readings differ by more than 20 % of the mean, repeat the determination.

## 7 Expression of results

### 7.1 Calculations

#### 7.1.1 Pigment portion of the liquid paint

Calculate the mass of "soluble" mercury in the hydrochloric acid extract obtained by the method described in sub-clause **8.2.3** of ISO 6713 using the equation

$$m_0 = \frac{a_1 - a_0}{10^6} \times \frac{V_1}{V_3} \times \frac{100}{5} \times F_1$$

$$= 2 \times 10^{-5} (a_1 - a_0) \frac{V_1}{V_3} \times F_1$$

where

$a_0$  is the mercury concentration, in micrograms per millilitres, of the blank test solution prepared by the method described in sub-clause **8.4** of ISO 6713;

$a_1$  is the mercury concentration, in micrograms per millilitre, of the test solution obtained from the calibration graph;

$F_1$  is the dilution factor referred to in **6.3.2**;

$m_0$  is the mass, in grams, of “soluble” mercury in the hydrochloric acid extract;

$V_1$  is the volume, in millilitres, of the hydrochloric acid plus ethanol used for the extraction described in sub-clause 8.2.3 of ISO 6713 (assumed to be 77 ml);

$V_3$  is the volume, in millilitres, of treated test solution pipetted into the reaction vessel according to 6.3.2.

Calculate the “soluble” mercury content of the pigment portion of the liquid paint, using the equation

$$C_{\text{Hg1}} = m_0 \times \frac{10^2}{m_1} \times \frac{P}{10^2} = \frac{m_0 \times P}{m_1}$$

where

$C_{\text{Hg1}}$  is the “soluble” mercury content, of the pigment portion of the liquid paint, expressed as a percentage by mass of the paint;

$m_1$  is the mass, in grams, of the test portion taken to prepare the solution described in sub-clause 8.2.3 of ISO 6713.

$P$  is the pigment content of the liquid paint, expressed as a percentage by mass, obtained by the appropriate method described in clause 6 of ISO 6713;

### 7.1.2 Liquid portion of the paint

Calculate the mass of mercury in the liquid portion of the paint (see 6.2.2) obtained according to 6.4.2 (method B) of ISO 6713 using the equation

$$m_2 = \frac{(b_1 - b_0) \times m_3 \times V_{\text{tot}} \times 100}{V_2 \times m_4} \times F_2$$

where

$b_0$  is the mercury concentration, in micrograms per millilitre, of the blank test solution (6.3.4);

$b_1$  is the mercury concentration, in micrograms per millilitre, of the test solution obtained from the calibration graph;

$F_2$  is the dilution factor referred to in 6.3.2;

$m_2$  is the mass, in grams, of mercury in the liquid portion of the paint;

$m_3$  is the total mass, in grams, of the non-volatile residue obtained according to 6.2.2.2;

$m_4$  is the mass, in grams, of the non-volatile residue test portion taken according to 6.2.2.3;

$V_{\text{tot}}$  is the total volume, in millilitres, of liquor prepared according to 6.2.2.1;

$V_2$  is the volume, in millilitres, of the solution obtained after the combustion (6.2.2.3).

Calculate the mercury content of the liquid portion of the paint using the equation

$$c_{\text{Hg2}} = \frac{m_2}{m_5} \times 10^2$$

where

$c_{\text{Hg2}}$  is the mercury content of the liquid portion of the paint, expressed as a percentage by mass of the paint;

$m_5$  is the total mass, in grams, of paint comprising a “set” as described in sub-clause 6.4 of ISO 6713.

### 7.1.3 Liquid paint

Calculate the total “soluble” mercury content of the liquid paint as the sum of the results obtained according to 7.1.1 and 7.1.2, thus

$$C_{\text{Hg3}} = C_{\text{Hg1}} + C_{\text{Hg2}}$$

where  $c_{\text{Hg3}}$  is the total “soluble” mercury content of the paint, expressed as a percentage by mass.

### 7.1.4 Paint in powder form

The total “soluble” mercury content of the paint in powder form is obtained by appropriate modification of the calculations given in 7.1.1.

### 7.1.5 Other test solutions

If the test solutions were prepared by methods other than those given in ISO 6713 (see 6.2.3), it will be necessary to modify the equations for the calculation of mercury content given in 7.1.1 and 7.1.2.

### 7.2 Precision

No precision data are currently available.


## 8 Test report


The test report shall contain at least the following information:

- the type and identification of the product tested;
- a reference to this International Standard (ISO 3856-7);
- the method for the separation of the solid portion of the product under test according to ISO 6713, clause 6 (method A, B or C), where appropriate<sup>3)</sup>;
- the solvent or the solvent mixture used for the extraction, where appropriate<sup>3)</sup>;

<sup>3)</sup> Not required for paints in powder form (see clause 7 of ISO 6713).

- e) the results of the test, expressed as a percentage by mass of the product: either
- the “soluble” mercury content of the pigment portion of the paint, the mercury content of the liquid portion of the paint and the total “soluble” mercury content of the liquid paint,
- or
- the total “soluble” mercury content of the paint in powder form;
- f) any deviation, by agreement or otherwise, from the test procedure specified;
- g) the date of the test.

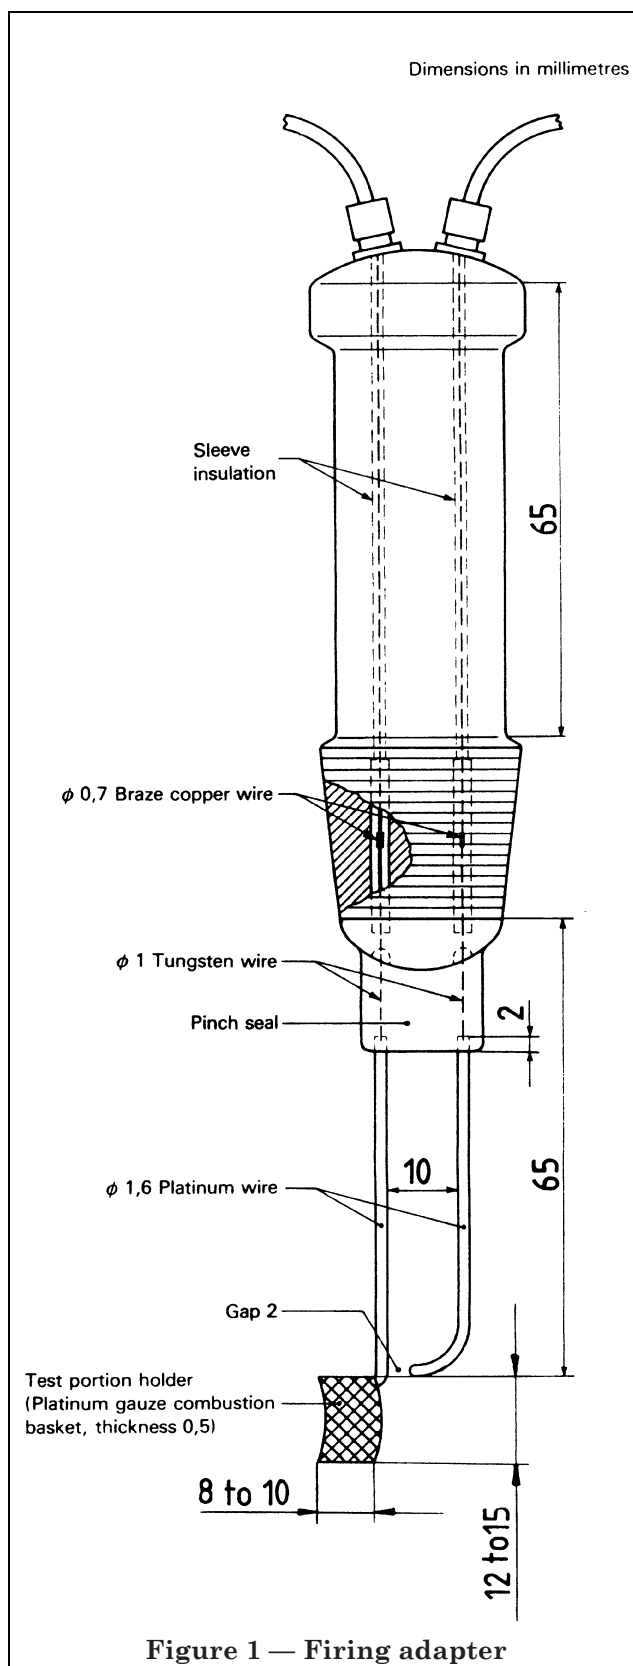

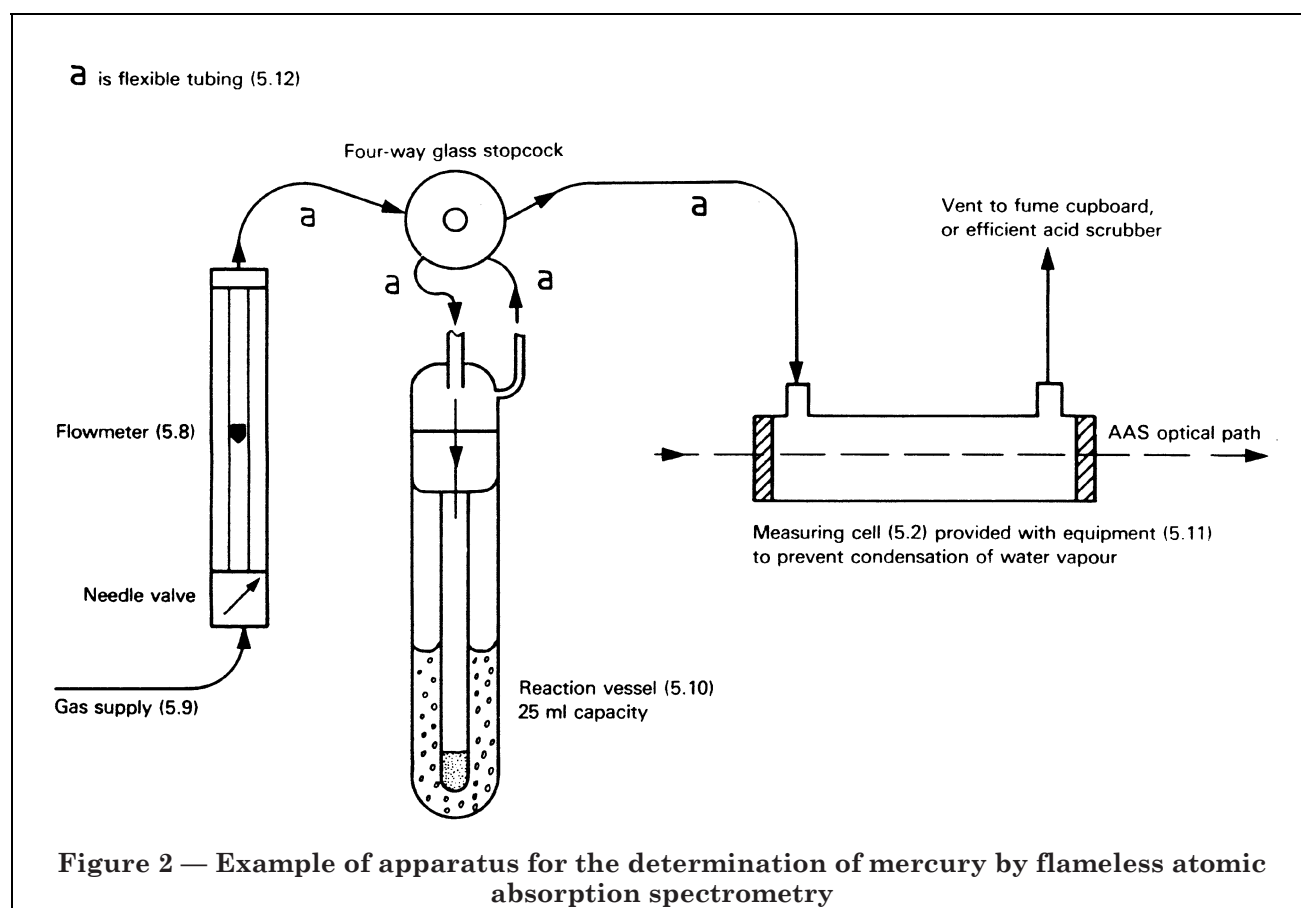

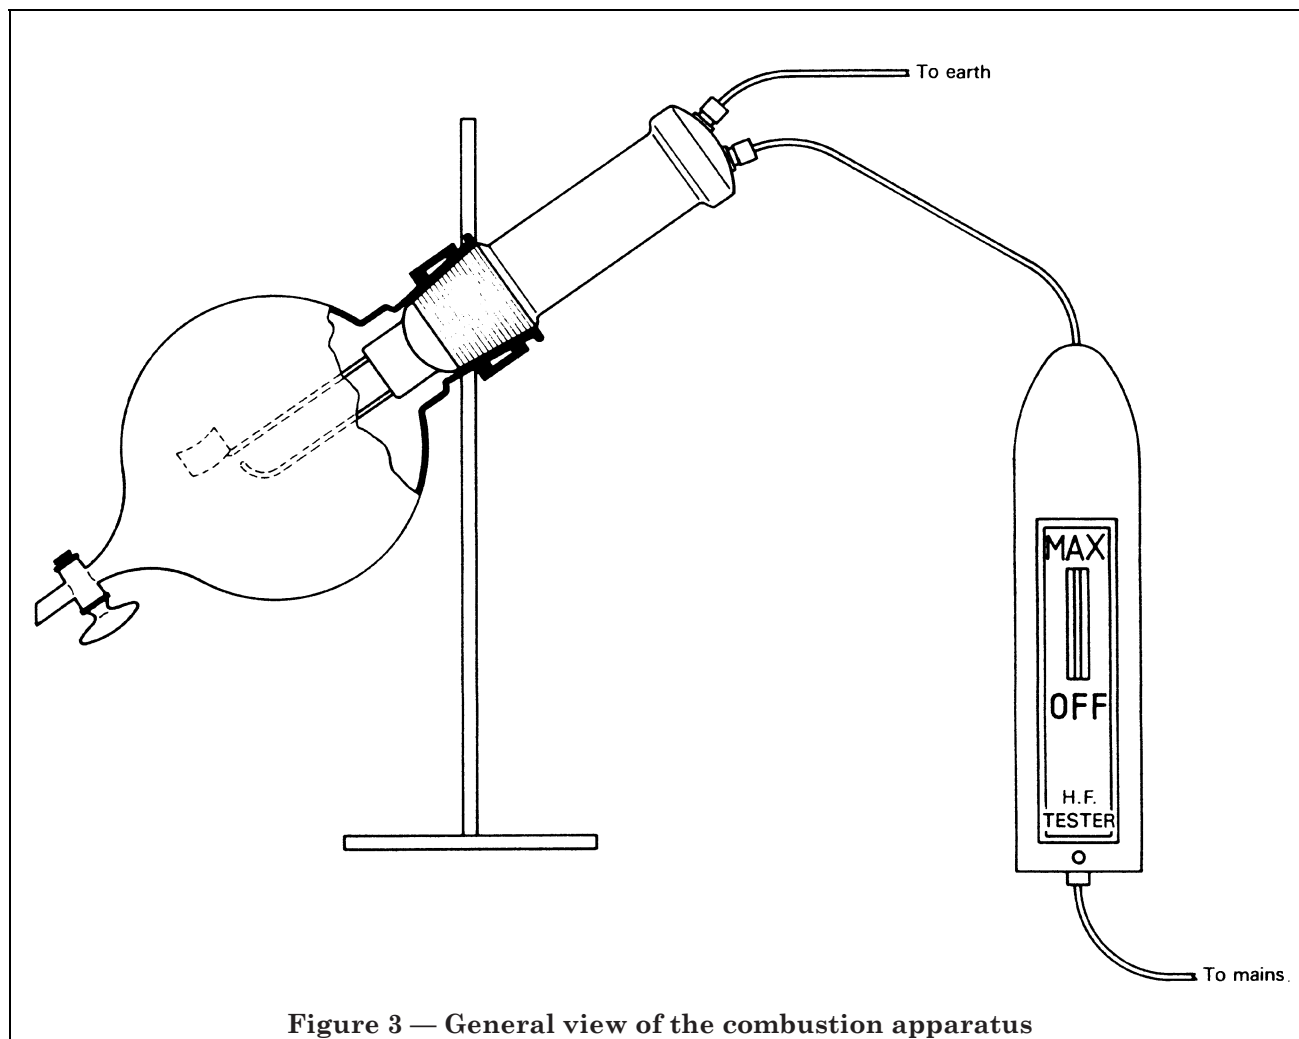


Figure 3 — General view of the combustion apparatus

## Publications referred to

See national foreword.



**BS 3900-B12:**  
**1986**  
**ISO 3856-7:**  
**1984**

---

# BSI — British Standards Institution

---

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

## Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

## Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

## Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

## Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.

BSI  
389 Chiswick High Road  
London  
W4 4AL